

# MIC Test Strip




### **Antimikrobiyal Duyarlılık Testi**

Minimum İnhibisyon Konsantrasyonunun belirlenmesine yönelik kantitatif test yöntemi (M.I.C.)


MIC Test Stripi antimikrobiyal ajanların mikroorganizmalara karşı minimum inhibisyon konsantrasyonunun (MIC) ve direnç mekanizmalarının belirlenmesine yönelik kantitatif bir test yöntemidir. MIC Test Stripleri patentli poroz yüzeyi üzerine antimikrobiyal ajan emdirilmiş striplerdir. Antimikrobiyal ajanın konsantrasyon aralığı geleneksel MIC metodundaki çift kat artan 15 farklı konsantrasyona karşılık gelmektedir.

Stribin bir yüzünde µg/mL biriminde bir MIC skalası ve antimikrobiyal ajanı tanımlayan kısaltma yer almaktadır. ESBL, MBL, GRD, AmpC ve KPC grubu mikroorganizmalar için iki farklı antimikrobiyal ajanın kullanıldığı çift yönlü stripler mevcuttur. Oldukça geniş bir antimikrobiyal ajan çeşitliliğine sahip olan **MIC Test Stripleri** 10, 30 ve 100 testlik ambalajlarda sunulmaktadır.

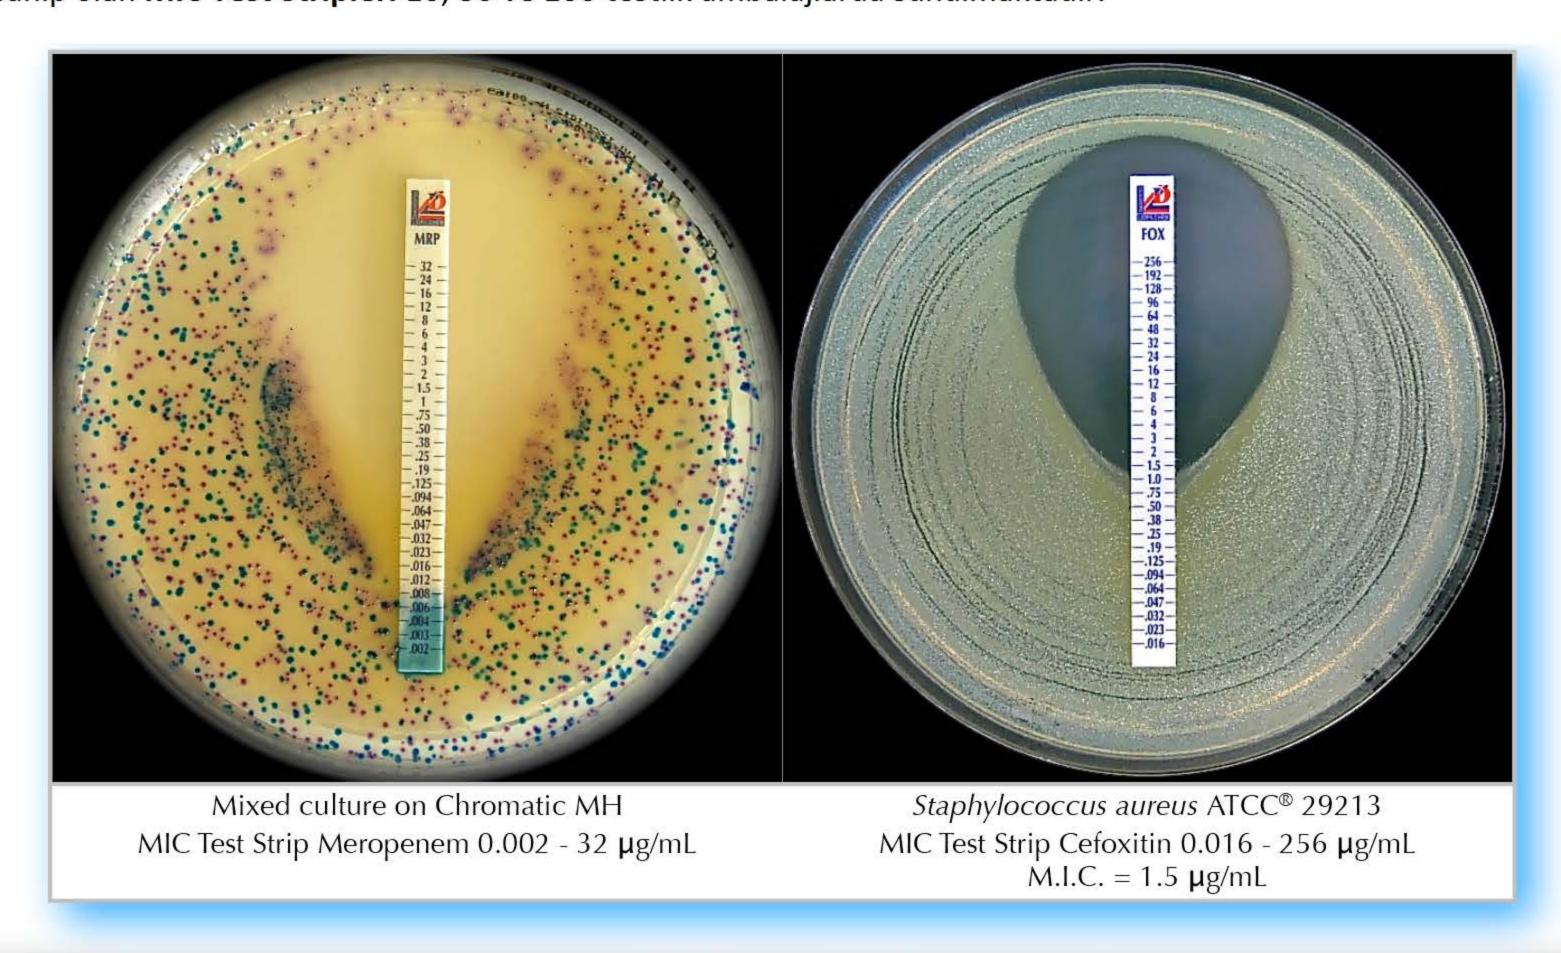


#### Metot prensibi

MIC Test Stribi inoküle edilmiş agar yüzeyine yerleştirildiği zaman antimikrobiyal ajan hızla ve strip boyunca artan konsantrasyonda agar matriksine difüze olur. 18 saat veya daha uzun inkübasyon sonrasında strip boyunca simetrik elips şeklinde bir inhibisyon zonu şekillenir. MIC değeri inhibisyon zonunun MIC Test Stribi ile keşistiği noktada strip üzerindeki skaladan μg/mL olarak okunabilir.

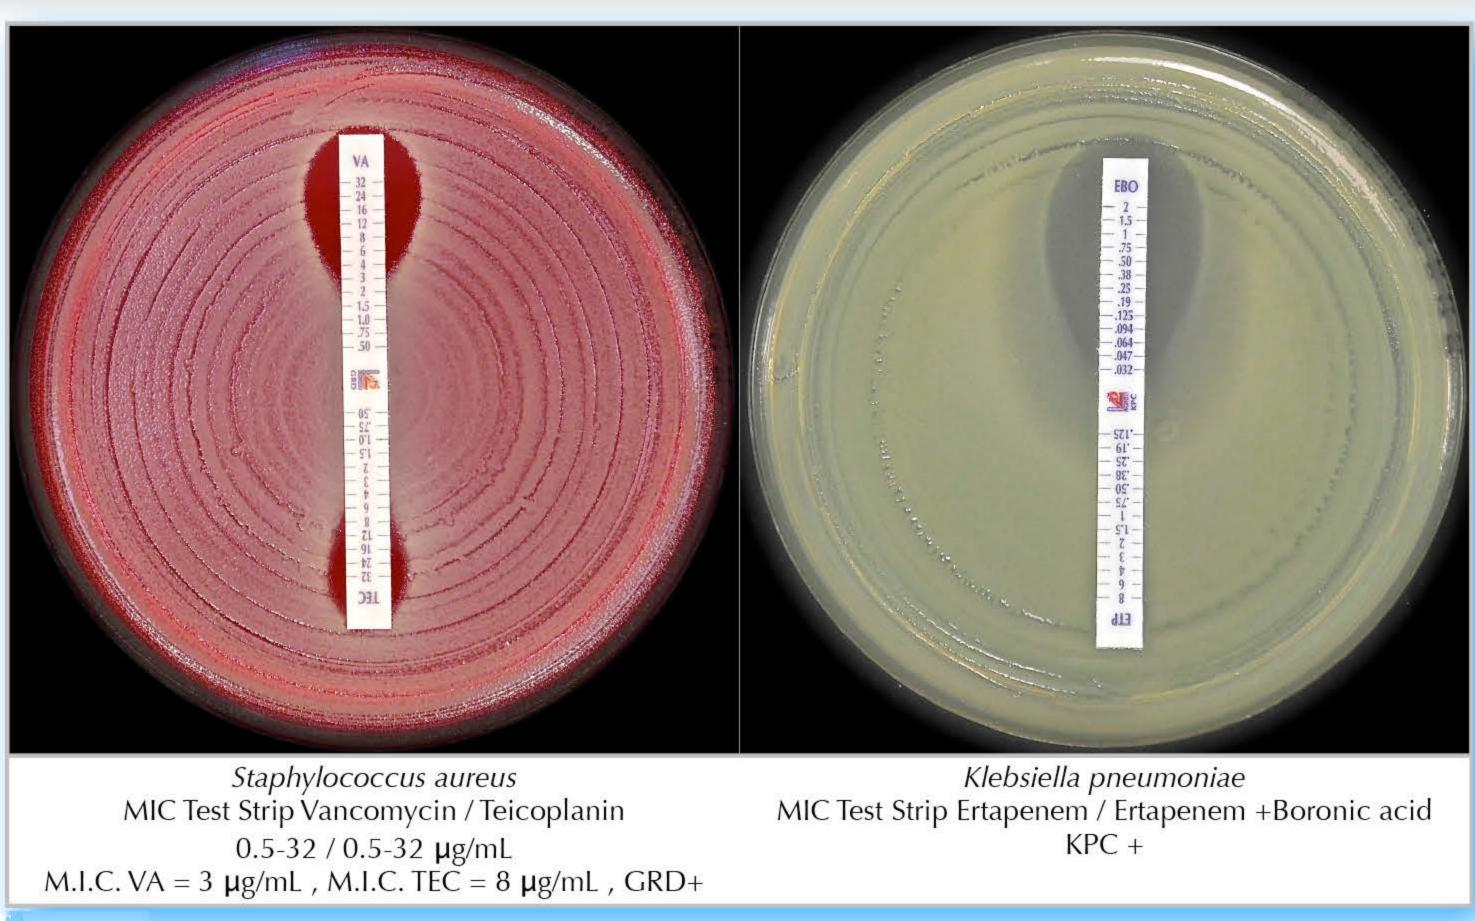

#### REFERANSLAR

- CLSI M100-S24, 2014. Performance Standards for Antimicrobial Susceptibility Testing.
- CLSI M7-A9, 2012. Methods for Dilution Antimicrobial Susceptibility Tests for Bacteria that Grow Aerobically.
- CLSI M11-A8 Methods for Antimicrobial Susceptibility Testing of Anaerobic Bacteria.
- CLSI M11-S1 Performance Standards for Antimicrobial Susceptibility Testing of Anaerobic Bacteria.
- CLSI M27-A3. Reference Method for Broth Dilution Antifungal Susceptibility Testing of Yeasts; Approved Standard Third Edition.
- CLSI M27-S4. Reference Method for Broth Dilution Antifungal Susceptibility Testing of Yeasts; Fourth Informational supplement.
- EUCAST. Breakpoint tables for interpretation of MICs and zone diameters Version 4.0, January 2014.

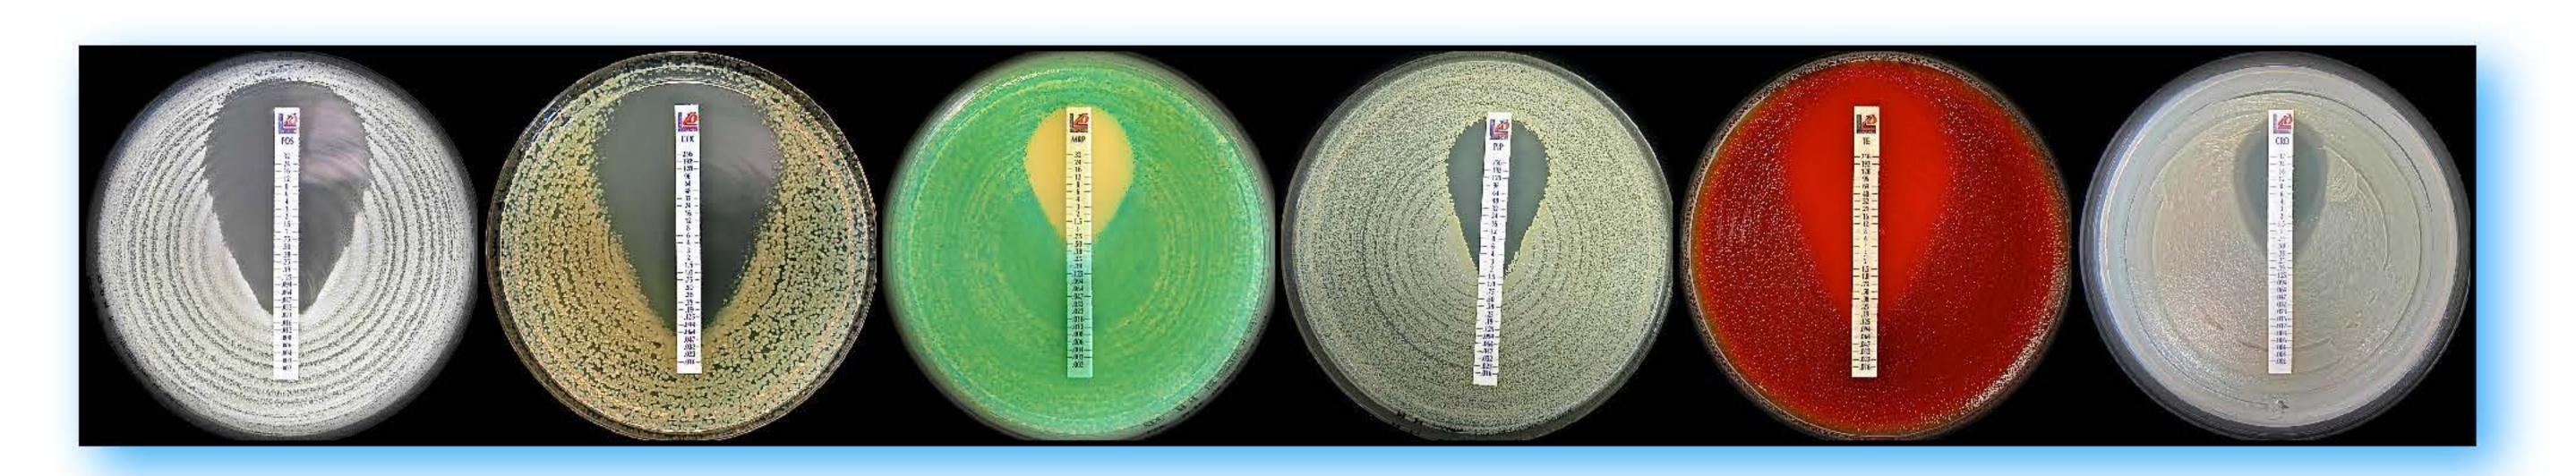

Description	Strip for ANTIMICROBIAL susceptible	/ Ο μg/mL	Code	Packaging	Ref
AIC Test Strip	AMIKACIN	0.016 - 256	AK	10 strips 30 strips	920181 92018
are resubtrip	AUVIINACIIN	0.010-230	ZXIX	100 strips	920180
HCT CL		0.046.056		10 strips	920211
11C Test Strip	AMOXICILLIN	0.016 - 256	AML	30 strips 100 strips	92021 920210
				100 strips	920241
AIC Test Strip	AMOXICILLIN*-CLAVULANIC ACID (2/1)  CLSI recommended	0.016 - 256*	AUG	30 strips	92024
·	CLSI recommended			100 strips	920240
HCT OF	AMOXICILLIN*-CLAVULANIC ACID (2 µg/ml)	0.046.056		10 strips	921801
4IC Test Strip	EUCAST recommended	0.016 - 256*	AMC	30 strips	92180
				100 strips 10 strips	921800 920031
AIC Test Strip	AMPICILLIN	0.016 - 256	AMP	30 strips	92003
				100 strips	920030
	AMPICILLIN*-SULBACTAM (2/1)			10 strips	920271
AIC Test Strip	CLSI recommended	0.016 - 256*	AMS	30 strips	92027
				100 strips	920270
AIC Test Strip	AMPICILLIN*-SULBACTAM (4 μg/mL)	0.016 - 256*	SAM	10 strips 30 strips	921811 92181
iic rest strip	EUCAST recommended	0.010 230	57 011	100 strips	921810
				10 strips	920301
AIC Test Strip	AZITHROMYCIN	0.016 - 256	AZM	30 strips	92030
				100 strips	920300
ALC TO LOCAL	A ZTDEONIANA	0.016.256	PARTEX A	10 strips	920331
4IC Test Strip	AZTREONAM	0.016 - 256	ATM	30 strips 100 strips	92033 920330
				100 strips	921731
AIC Test Strip	AZTREONAM	0.064 - 1024	ATM	30 strips	92173
				100 strips	921730
				10 strips	920191
4IC Test Strip	BACITRACIN	0.016 - 256	BA	30 strips	92019
				100 strips	920190
AIC Tost Strip	CEFACLOR	0.016 - 256	CEC	10 strips	920361 92036
AIC Test Strip	CEFACLOR	0.016 - 236	CEC	30 strips 100 strips	920360
				10 strips	921261
AIC Test Strip	CEFEPIME	0.016 - 256	FEP	30 strips	92126
				100 strips	921260
W.C.T			ee.	10 strips	920601
4IC Test Strip	CEFIXIME	0.016 - 256	CFM	30 strips	92060
				100 strips 10 strips	920600 920231
AIC Test Strip	CEFOPERAZONE*-SULBACTAM (2/1)	0.016 - 256*	CPS	30 strips	920231
			17/18 37/1	100 strips	920230
				10 strips	920071
AIC Test Strip	CEFOTAXIME	0.002 - 32	CTX	30 strips	92007
				100 strips	920070
AIC Tost Strip	CEFOTAXIME	0.016 - 256	CTV	10 strips	920061
4IC Test Strip	CEPOTAXIME	0.016 - 236	CTX	30 strips 100 strips	92006 920060
				10 strips	920201
AIC Test Strip	CEFOTETAN	0.016 - 256	CTT	30 strips	92020
				100 strips	920200
				10 strips	920661
11C Test Strip	CEFOXITIN	0.016 - 256	FOX	30 strips	92066
				100 strips	920660
11C Test Strip	CEFPIROME	0.016 - 256	CR	10 strips 30 strips	920081 92008
ine resulting	CELLINCHAE	0.010 - 230	CIX	100 strips	920080
				10 strips	920051
AIC Test Strip	CEFPODOXIME	0.016 - 256	PX	30 strips	92005
				100 strips	920050
HCT . C. I	CEETADO LINE	0.046.056	CDT	10 strips	920491
1IC Test Strip	CEFTAROLINE	0.016 - 256	CPT	30 strips	92049 920490
				100 strips 10 strips	920490 921381
11C Test Strip	CEFTAZIDIME	0.016 - 256	CAZ	30 strips	92138
Υ. Ε				100 strips	921380
				10 strips	920581
11C Test Strip	CEFTIBUTEN	0.002 - 32	CTB	30 strips	92058
				100 strips	920580
ALC Took Stales	CEETIZOVIA 4E	0.000 22	CZV	10 strips	920161
11C Test Strip	CEFTIZOXIME	0.002 - 32	CZX	30 strips 100 strips	92016 920160
				10 strips	920421
IIC Test Strip	CEFTRIAXONE	0.016 - 256	CRO	30 strips	92042
				100 strips	920420

	Strip for ANTIMICROBIAL susceptib	<i>y</i>			D . C
Description		µg/mL	Code	Packaging 10 strips	<b>Ref.</b> 920431
MIC Test Strip	CEFTRIAXONE	0.002 - 32	CRO	30 strips 100 strips	92043 920430
MIC Test Strip	CEFUROXIME	0.016 - 256	CXM	10 strips 30 strips 100 strips	921291 92129 921290
MIC Test Strip	CEPHALOTHIN	0.016 - 256	KF	10 strips 30 strips 100 strips	920391 92039 920390
MIC Test Strip	CHLORAMPHENICOL	0.016 - 256	С	10 strips 30 strips 100 strips	920751 92075 920750
MIC Test Strip	CIPROFLOXACIN	0.002 - 32	CIP	10 strips 30 strips	920451 92045
MIC Test Strip	CLARITHROMYCIN	0.016 - 256	CLR	100 strips 10 strips 30 strips	920450 920481 92048
MIC Test Strip	CLINDAMYCIN	0.016 - 256	CD	100 strips 10 strips 30 strips	920480 920721 92072
MIC Test Strip	CLOXACILLIN	0.016 - 256	CX	100 strips 10 strips 30 strips	920720 920441 92044
MIC Test Strip	COLISTIN	0.016 - 256	CS	100 strips 10 strips 30 strips	920440 921411 92141
				100 strips 10 strips	921410 921421
MIC Test Strip	COLISTIN	0.064 - 1024	CS	30 strips 100 strips 10 strips	92142 921420 921451
MIC Test Strip	DAPTOMYCIN (Includes Ca <sup>2+</sup> )	0.016 - 256	DAP	30 strips 100 strips	92145 921450
MIC Test Strip	DORIPENEM	0.002 - 32	DOR	10 strips 30 strips 100 strips	920401 92040 920400
MIC Test Strip	DOXYCYCLINE	0.016 - 256	DXT	10 strips 30 strips 100 strips	921561 92156 921560
MIC Test Strip	ENROFLOXACIN	0.002 - 32	ENR	10 strips 30 strips 100 strips	920131 92013 920130
MIC Test Strip	ERTAPENEM	0.002 - 32	ETP	10 strips 30 strips 100 strips	921571 92157 921570
MIC Test Strip	ERYTHROMYCIN	0.016 - 256	E	10 strips 30 strips 100 strips	920511 92051 920510
MIC Test Strip	FOSFOMYCIN (Includes Glucose-6-Phosphate)	0.016 - 256	FOS	10 strips 30 strips 100 strips	920781 92078 920780
MIC Test Strip	FOSFOMYCIN (Includes Glucose-6-Phosphate)	0.064 - 1024	FOS	10 strips 30 strips 100 strips	920791 92079 920790
MIC Test Strip	FUSIDIC ACID	0.016 - 256	FU	10 strips 30 strips	920021 92002
MIC Test Strip	GATIFLOXACIN	0.002 - 32	GAT	100 strips 10 strips 30 strips	920020 920111 92011
MIC Test Strip	GEMIFLOXACIN	0.002 - 32	GEM	100 strips 10 strips 30 strips	920110 920351 92035
MIC Test Strip	GENTAMICIN	0.016 - 256	CN	100 strips 10 strips 30 strips	920350 920091 92009
MIC Test Strip	GENTAMICIN	0.064 - 1024	CN	100 strips 10 strips 30 strips	920090 920101 92010
				100 strips 10 strips	920100 920541
MIC Test Strip	IMIPENEM	0.002 - 32	IMI	30 strips 100 strips 10 strips	92054 920540 920341
MIC Test Strip	KANAMYCIN	0.016 - 256	K	30 strips 100 strips 10 strips	92034 920340 920811
MIC Test Strip	LEVOFLOXACIN	0.002 - 32	LEV	30 strips 100 strips 10 strips	92081 920810 921351
MIC Test Strip	LINEZOLID	0.016 - 256	LNZ	30 strips 100 strips	92135 921350
MIC Test Strip	MECILLINAM	0.016 - 256	MEC	10 strips 30 strips 100 strips	920171 92017 920170
MIC Test Strip	MEROPENEM	0.002 - 32	MRP	10 strips 30 strips 100 strips	920841 92084 920840
MIC Test Strip	METRONIDAZOLE	0.016 - 256	MTZ	10 strips 30 strips 100 strips	920871 92087 920870

Description	t Strip for ANTIMICROBIAL suscepti	phity testing µg/mL	Code	Packaging	Re
MIC Test Strip	MOXIFLOXACIN	0.002 - 32	MXF	10 strips 30 strips 100 strips	92090 92090 92090
MIC Test Strip	MUPIROCIN	0.064 - 1024	MUP	10 strips 30 strips 100 strips	92038 92038 92038
MIC Test Strip	MINOCYCLINE	0.016 - 256	MN	10 strips 30 strips 100 strips	92032 92032 92032
MIC Test Strip	NALIDIXIC ACID	0.016 - 256	NA	10 strips 30 strips 100 strips	92132 92132 92132
MIC Test Strip	NETILMICIN	0.016 - 256	NET	10 strips 30 strips 100 strips	92093 92093 92093
MIC Test Strip	NORFLOXACIN	0.016 - 256	NOR	10 strips 30 strips 100 strips	92096 92096 92096
MIC Test Strip	NITROFURANTOIN	0.032 - 512		10 strips 30 strips 100 strips	92022 92022 92022
MIC Test Strip	OFLOXACIN	0.002 - 32	OFX	10 strips 30 strips 100 strips	92099 92099 92099
MIC Test Strip	OXACILLIN	0.016 - 256	ОХ	10 strips 30 strips 100 strips	92015 92015 92015
MIC Test Strip	PENICILLIN G	0.002 - 32	Р	10 strips 30 strips 100 strips	92103 92103 92103
MIC Test Strip	PENICILLIN G	0.016 - 256	Р	10 strips 30 strips 100 strips	92102 92102 92102
MIC Test Strip	PIPERACILLIN	0.016 - 256	PIP	10 strips 30 strips 100 strips	92105 92105 92105
MIC Test Strip	PIPERACILLIN*-TAZOBACTAM (4 μg/mL)	0.016 - 256*	TZP	10 strips 30 strips 100 strips	92108 92108 92108
MIC Test Strip	POLYMYXIN B	0.064 - 1024	РВ	10 strips 30 strips 100 strips	92004 92004 92004
MIC Test Strip	QUINUPRISTIN-DALFOPRISTIN	0.002 - 32	QDA	10 strips 30 strips 100 strips	92026 92026 92026
MIC Test Strip	RIFAMPICIN	0.002 - 32	RD	10 strips 30 strips 100 strips	9200° 9200° 9200°
MIC Test Strip	RIFAMPICIN	0.016 - 256	RD	10 strips 30 strips 100 strips	92025 92025 92025
MIC Test Strip	SPECTINOMYCIN	0.064 - 1024	SPC	10 strips 30 strips 100 strips	92014 92014 92014
MIC Test Strip	SPIRAMYCIN	0.002 - 32	SP	10 strips 30 strips 100 strips	92046 92046 92046 9211
MIC Test Strip	STREPTOMYCIN	0.064 - 1024	S	10 strips 30 strips 100 strips 10 strips	92111 92111 92111 92028
MIC Test Strip	SULBACTAM	0.016 - 256	SUL	30 strips 100 strips 100 strips	92028 92028 92031
MIC Test Strip	SULFAMETHOXAZOLE	0.064 - 1024	SMX	30 strips 100 strips 10 strips	92031 92031 92012
MIC Test Strip	TEICOPLANIN	0.016 - 256	TEC	30 strips 100 strips 10 strips	92012 92012 92052
MIC Test Strip	TELAVANCIN	0.002 - 32	TLV	30 strips 100 strips 10 strips	92052 92052 92053
MIC Test Strip	TELAVANCIN	0.016 - 256	TLV	30 strips 100 strips 10 strips	92053 92053 92029
MIC Test Strip	TEMOCILLIN	0.064 - 1024	TMO	30 strips 100 strips 10 strips	92029 92029 92114
MIC Test Strip	TETRACYCLINE	0.016 - 256	TE	30 strips 100 strips 10 strips	9211 <sup>2</sup> 9211 <sup>2</sup> 92200
MIC Test Strip	TIAMULIN	0.002 - 32	TIA	30 strips 100 strips 10 strips	92200 92200 92112
MIC Test Strip	TICARCILLIN*-CLAVULANIC ACID (2 μg/mL)	0.016 - 256*	TTC	30 strips 100 strips 10 strips	92117 92117 92144
MIC Test Strip	TIGECYCLINE	0.016 - 256	TGC	30 strips 100 strips	92144 92144

MIC Test	MIC Test Strip for ANTIMICROBIAL susceptibility testing						
Description		μg/mL	Code	Packaging	Ref.		
MIC Test Strip	TILMICOSIN	0.002 - 32	TIL	10 strips 30 strips 100 strips	922011 92201 922010		
MIC Test Strip	TOBRAMYCIN	0.016 - 256	ТОВ	10 strips 30 strips 100 strips	921211 92121 921210		
MIC Test Strip	TOBRAMYCIN	0.064 - 1024	ТОВ	10 strips 30 strips 100 strips	921201 92120 921200		
MIC Test Strip	TRIMETHOPRIM	0.002 - 32	TM	10 strips 30 strips 100 strips	920371 92037 920370		
MIC Test Strip	TRIMETHOPRIM*-SULFAMETHOXAZOLE (1/19)	0.002 - 32*	SXT	10 strips 30 strips 100 strips	921231 92123 921230		
MIC Test Strip	VANCOMYCIN	0.016 - 256	VA	10 strips 30 strips 100 strips	920571 92057 920570		

POS

MIC Test	Strip for ANTIFUNC	GAL susceptibility testing			
Description		μg/mL	Code	Packaging	Ref.
MIC Test Strip	amphotericin b	0.002 - 32	AMB	10 strips 30 strips 100 strips	921531 92153 921530
MIC Test Strip	ANIDULAFUNGIN	0.002 - 32	AND	10 strips 30 strips 100 strips	921551 92155 921550
MIC Test Strip	CASPOFUNGIN	0.002 - 32	CAS	10 strips 30 strips 100 strips	921541 92154 921540
MIC Test Strip	fluconazole	0.016 - 256	FLU	10 strips 30 strips 100 strips	921471 92147 921470
MIC Test Strip	FLUCYTOSINE	0.002 - 32	FC	10 strips 30 strips 100 strips	921491 92149 921490
MIC Test Strip	ITRACONAZOLE	0.002 - 32	ITC	10 strips 30 strips 100 strips	921481 92148 921480
MIC Test Strip	KETOCONAZOLE	0.002 - 32	KE	10 strips 30 strips 100 strips	921511 92151 921510
MIC Test Strip	MICAFUNGIN	0.002 - 32	MYC	10 strips 30 strips 100 strips	921821 92182 921820
MIC Test Strip	POSACONAZOLE	0.002 - 32	POS	10 strips 30 strips 100 strips	921521 92152 921520
MIC Test Strip	Voriconazole	0.002 - 32	VO	10 strips 30 strips 100 strips	921501 92150 921500

MIC Test Strip for ANTIMYCOBACTERIAL susceptibility testing						
Description		µg/mL	Code	Packaging	Ref.	
				10 strips	921701	
MIC Test Strip	ETHAMBUTOL	0.016 - 256	EB	30 strips	92170	
				100 strips	921700	
				10 strips	921721	
MIC Test Strip	ETHIONAMIDE	0.016 - 256	ET	30 strips	92172	
				100 strips	921720	
				10 strips	921711	
MIC Test Strip	ISONIAZIDE	0.016 - 256	IZ	30 strips	92171	
				100 strips	921710	

MIC Test Strip ESBL for confirmation of Extended Spectrum Beta-Lactamase							
Description		μg/mL	Code	Packaging	Ref.		
				10 strips	921611		
MIC Test Strip	CEFEPIME/CEFEPIME+CLAVULANIC ACID (4 µg/mL)	0.25-16 / 0.064-4	FEP/FEL	30 strips	92161		
				100 strips	921610		
				10 strips	921601		
MIC Test Strip	CEFOTAXIME/CEFOTAXIME+CLAVULANIC ACID (4 µg/ml)	0.25-16 / 0.016-1	CTX/CTL	30 strips	92160		
2.				100 strips	921600		
				10 strips	921591		
MIC Test Strip	CEFTAZIDIME/CEFTAZIDIME+CLAVULANIC ACID (4 µg/ml)	0.5-32 / 0.064-4	CAZ/CAL	30 strips	92159		
	THE THE PERSON OF THE PERSON AND PERSON WITH THE PERSON AND PERSON AND PERSON OF THE P			100 strips	921590		

MIC Test	Strip for <b>KPC</b> detection				
Description		μg/mL	Code	Packaging	Ref.
				10 strips	921671
MIC Test Strip	MEROPENEM / MEROPENEM + BORONIC ACID	0.125-8/0.032-2	MRP/MBO	30 strips	92167
				100 strips	921670
				10 strips	921681
<b>MIC Test Strip</b>	ertapenem / ertapenem + boronic acid	0.125-8/0.032-2	ETP/EBO	30 strips	92168
lint.				100 strips	921680

MIC Test Strip MBL for detection of Metallo Beta-Lactamase							
Description		µg/mL	Code	Packaging	Ref.		
				10 strips	921621		
MIC Test Strip	IMIPENEM / IMIPENEM + EDTA	4-256 / 1-64	IMI/IMD	30 strips	92162		
· ·				100 strips	921620		
12				10 strips	921661		
MIC Test Strip	IMIPENEM / IMIPENEM + EDTA	0.125-8 / 0.032-2	IMI/IMD	30 strips	92166		
				100 strips	921660		
				10 strips	921651		
MIC Test Strip	MEROPENEM / MEROPENEM + EDTA	0.125-8 / 0.032-2	MRP/MRD	30 strips	92165		
				100 strips	921650		


MIC Test Strip GRD for detection of Glycopeptide Resistance investigational use only					
Description		µg/mL	Code	Packaging	Ref.
				10 strips	921631
MIC Test Strip	VANCOMYCIN / TEICOPLANIN	0.5-32 / 0.5-32	<b>VA/TEC</b>	30 strips	92163
				100 strips	921630


MIC Test	Strip for AmpC detection	investigational use only			
Description		μg/mL	Code	Packaging	Ref.
MIC Test Strip	CEFOTETAN / CEFOTETAN+CLOXACILLIN	0.5-32 / 0.5-32	CTT/CXT	10 strips 30 strips 100 strips	921641 92164 921640
MIC Test Strip	ertapenem / ertapenem + cloxacillin	0.125-8 / 0.032-2	ETP/ECX	10 strips 30 strips 100 strips	921691 92169 921690


MTS Synergy Application System (patent	pending)	
Description	Packaging	Ref.
MTS Synergy Applicator Platform	1 unit	96860
MTS Synergy Delivery Tool	10 disposab applicators	le 96870


Accessories			
Description		Packaging	Ref.
Automatic Rotation Plater 90 mm plates 14-110 rpm		1 unit	96795
Automatic Rotation Plater PRO (14-210 rpm)		1 unit	96796
Turntable extra wide (140 mm plates)		1 unit	96797
Wireless Foot Pedal		1 unit	96801
Steel Foot Pedal		1 unit	96798
Plastic Foot Pedal		1 unit	96799
STORAGE TUBE WITH SILICA GEL	CTV	10 tubes	96719
0.5 McFarland	1-16	1 tube	80400
1 McFarland	12	1 tube	80401
2 McFarland	1 8	1 tube	80402

Ready to use culture media			
DESCRIPTION	FORMAT	PACKAGING	REF.
MUELLER HINTON AGAR II for antimicrobial susceptibility testing of non-fastidious organisms.	90 mm 140 mm	20 plates 10 plates	10031 10231
MUELLER HINTON AGAR II + SHEEP BLOOD 5% for antimicrobial susceptibility testing of fastidious organisms.	90 mm 140 mm	20 plates 10 plates	10131 11231
MUELLER HINTON FASTIDIOUS AGAR (Horse blood 5% + 20 mg/L $\beta$ -NAD) EUCAST recommended: for antimicrobial susceptibility testing of <i>Streptococcus</i> spp., <i>Haemophilus</i> spp., and some other fastidious organisms.	90 mm 140 mm	20 plates 10 plates	10132 11132
MUELLER HINTON AGAR II + 2% NaCl for antimicrobial susceptibility testing of staphylococci with Oxacillin.	90 mm	20 plates	11206
CHROMATIC MH Chromogenic medium for the preliminary identification and susceptibility testing of bacteria directly from clinical and environmental specimens.	90 mm	20 plates	11618
BRUCELLA BLOOD AGAR with HEMIN AND VITAMIN K1 for antimicrobial susceptibility testing of anaerobic bacteria.	90 mm	20 plates	10245
SCHADLER K AGAR (SHEEP BLOOD 5%) for antimicrobial susceptibility testing of anaerobic bacteria.	90 mm	20 plates	11065
HAEMOPHILUS TEST AGAR for <i>Haemophilus</i> spp. susceptibility testing.	90 mm	20 plates	10080
MIDDLEBROOK 7H11 AGAR for antimicrobial susceptibility testing of mycobacteria.	90 mm	20 plates	10416
R.P.M.I. AGAR (2% glucose + MOPS) for antifungal susceptibility testing.	90 mm 140 mm	20 plates 10 plates	11509 10233

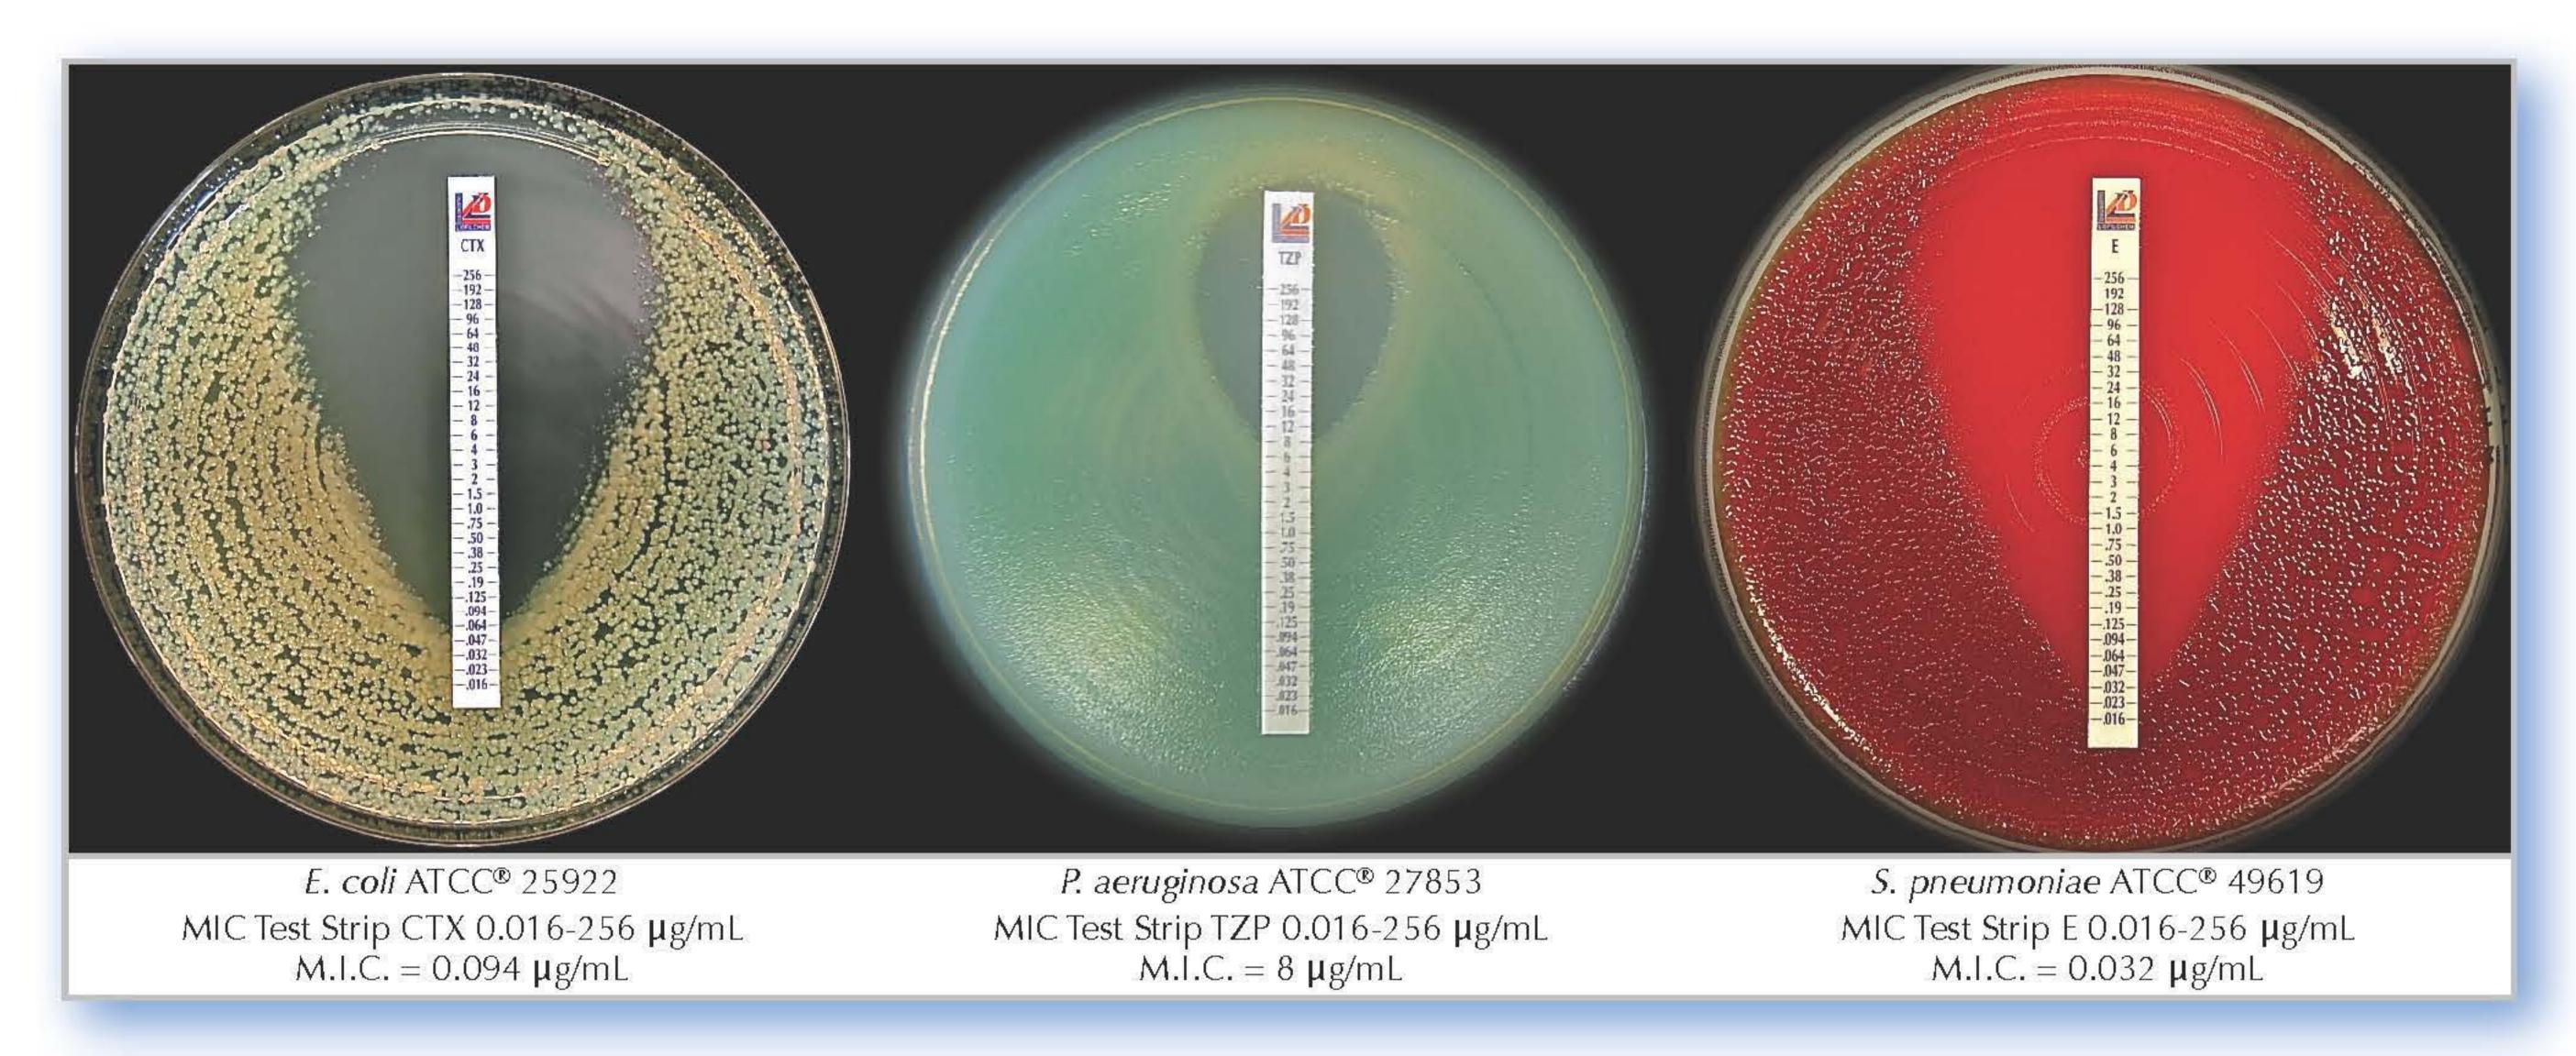

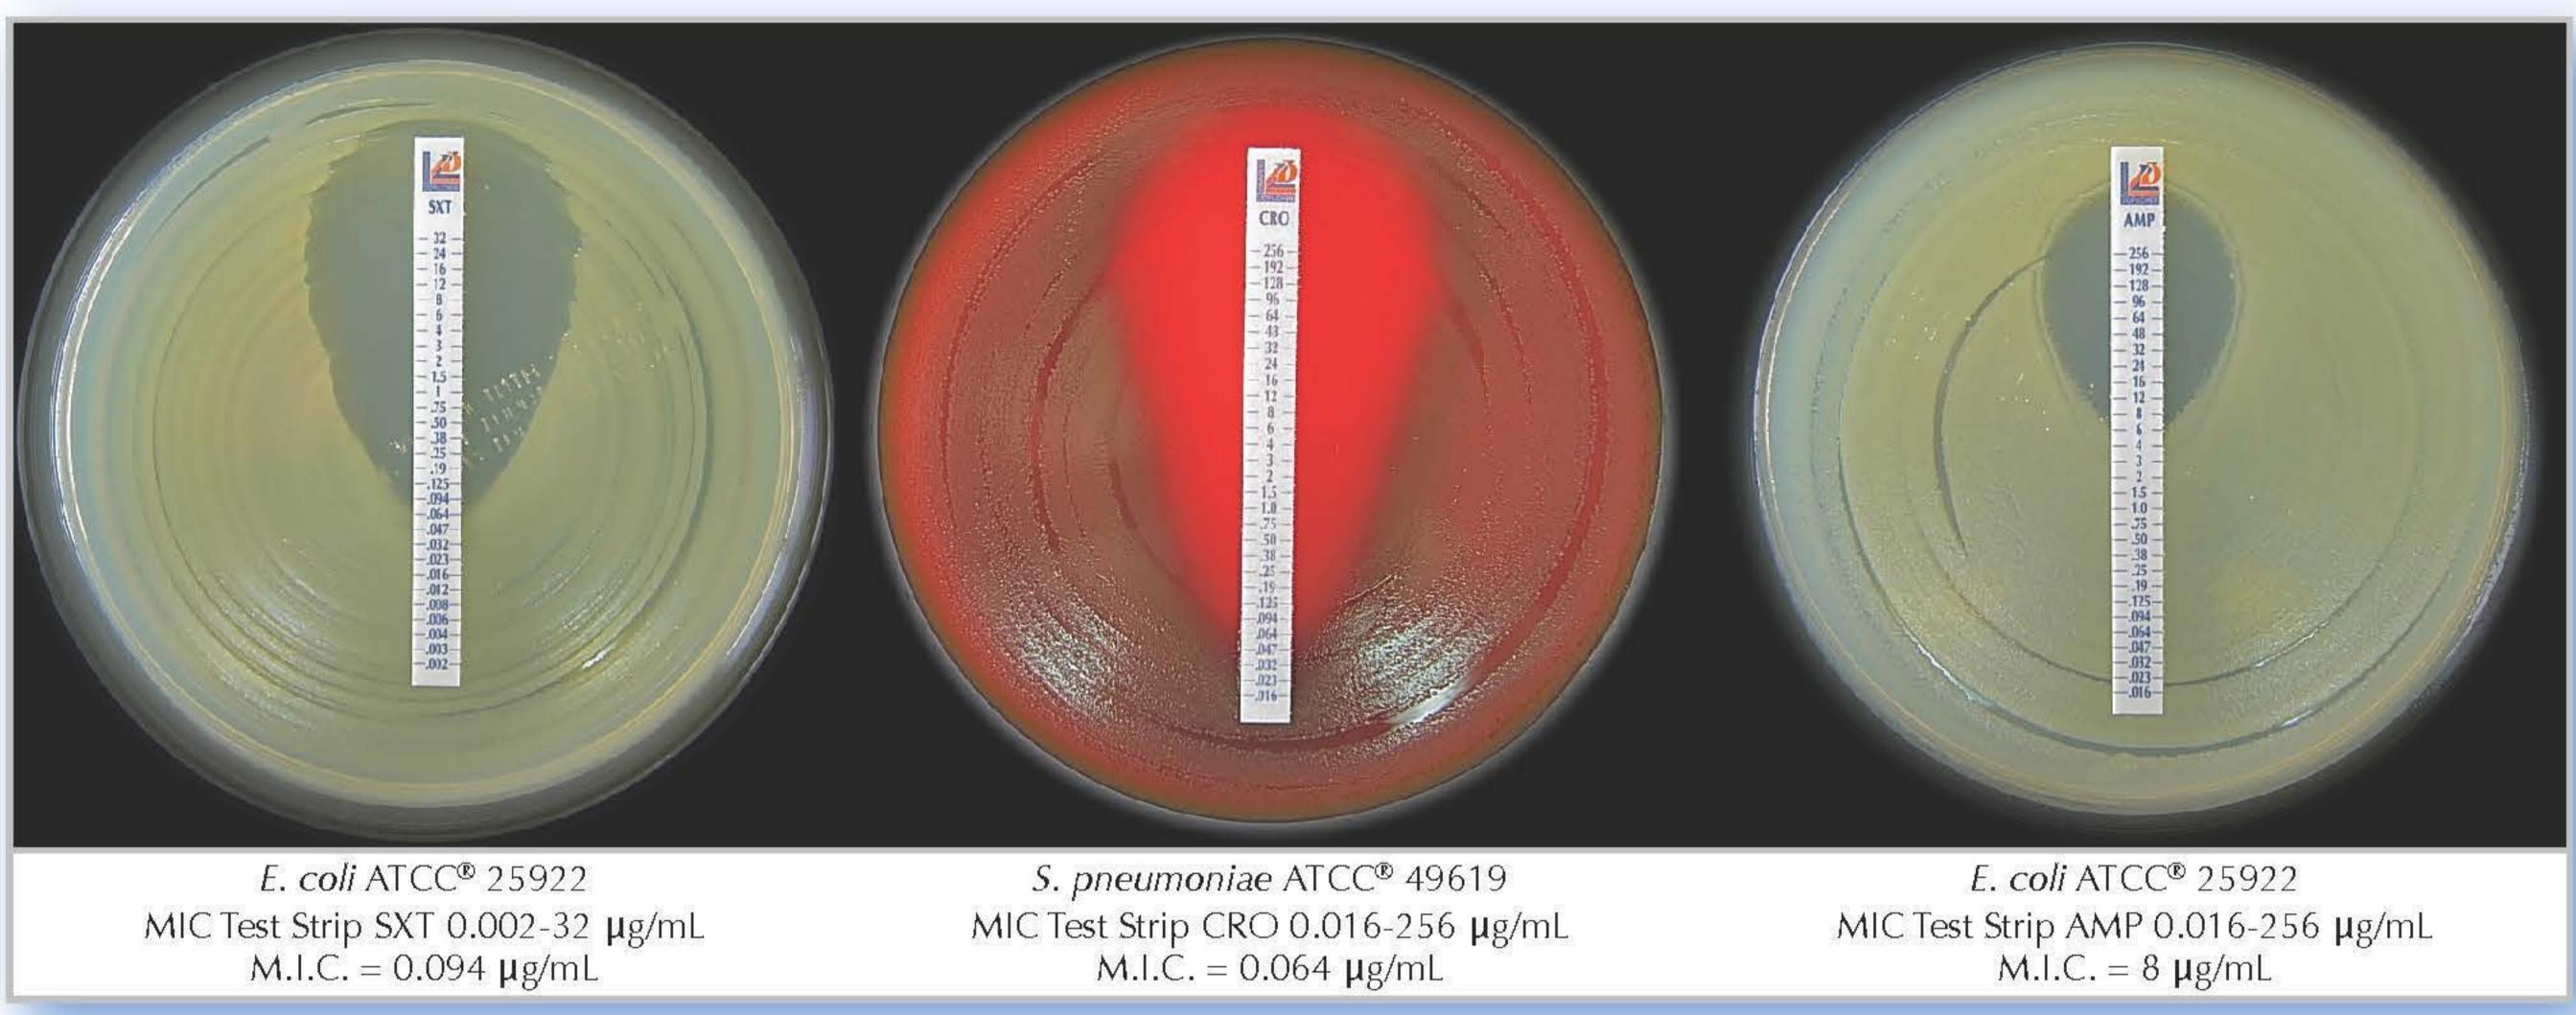

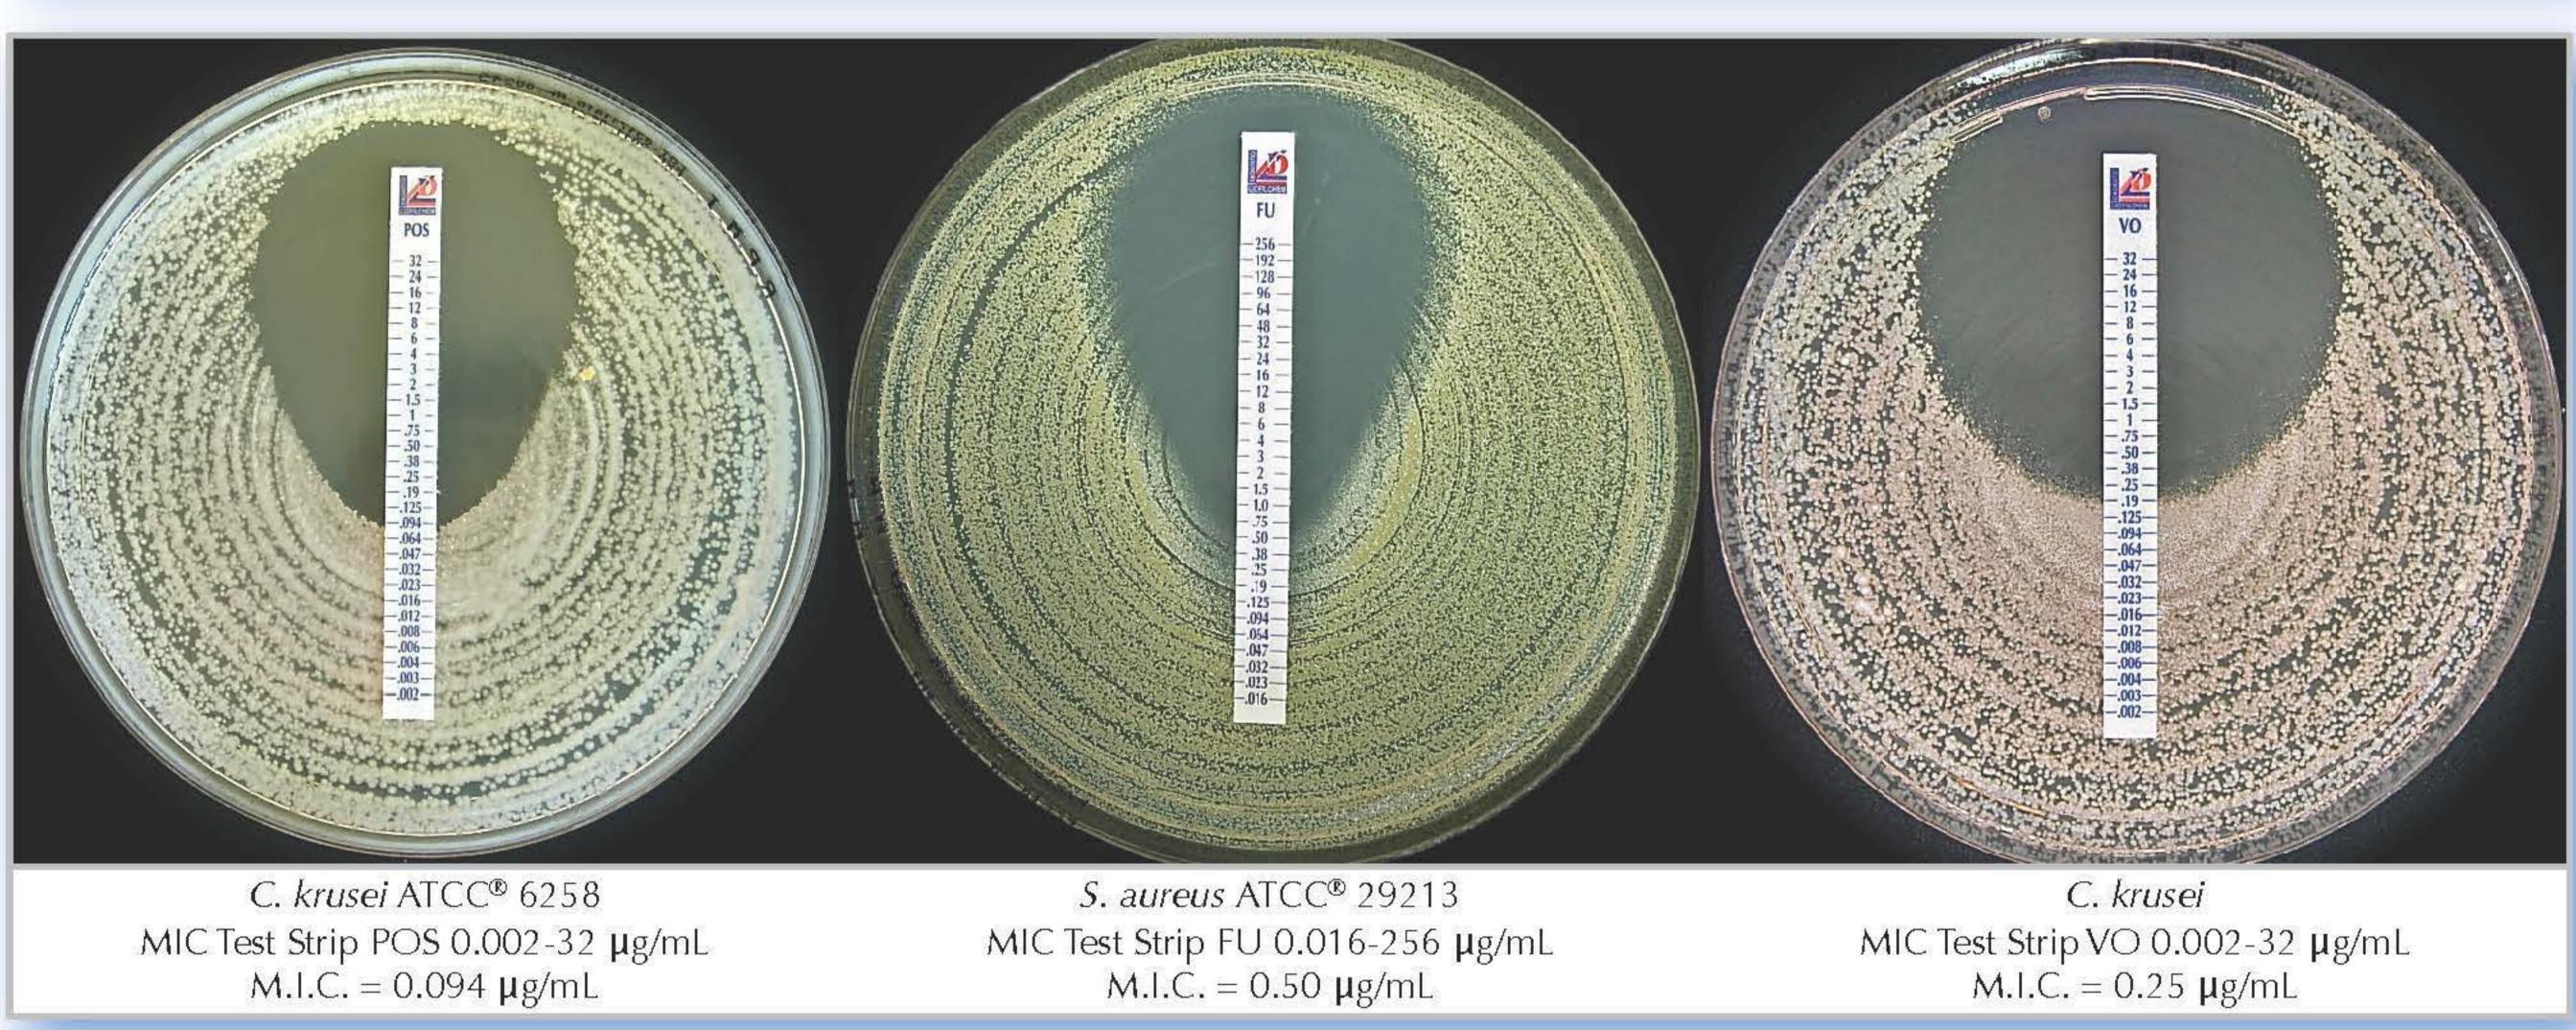

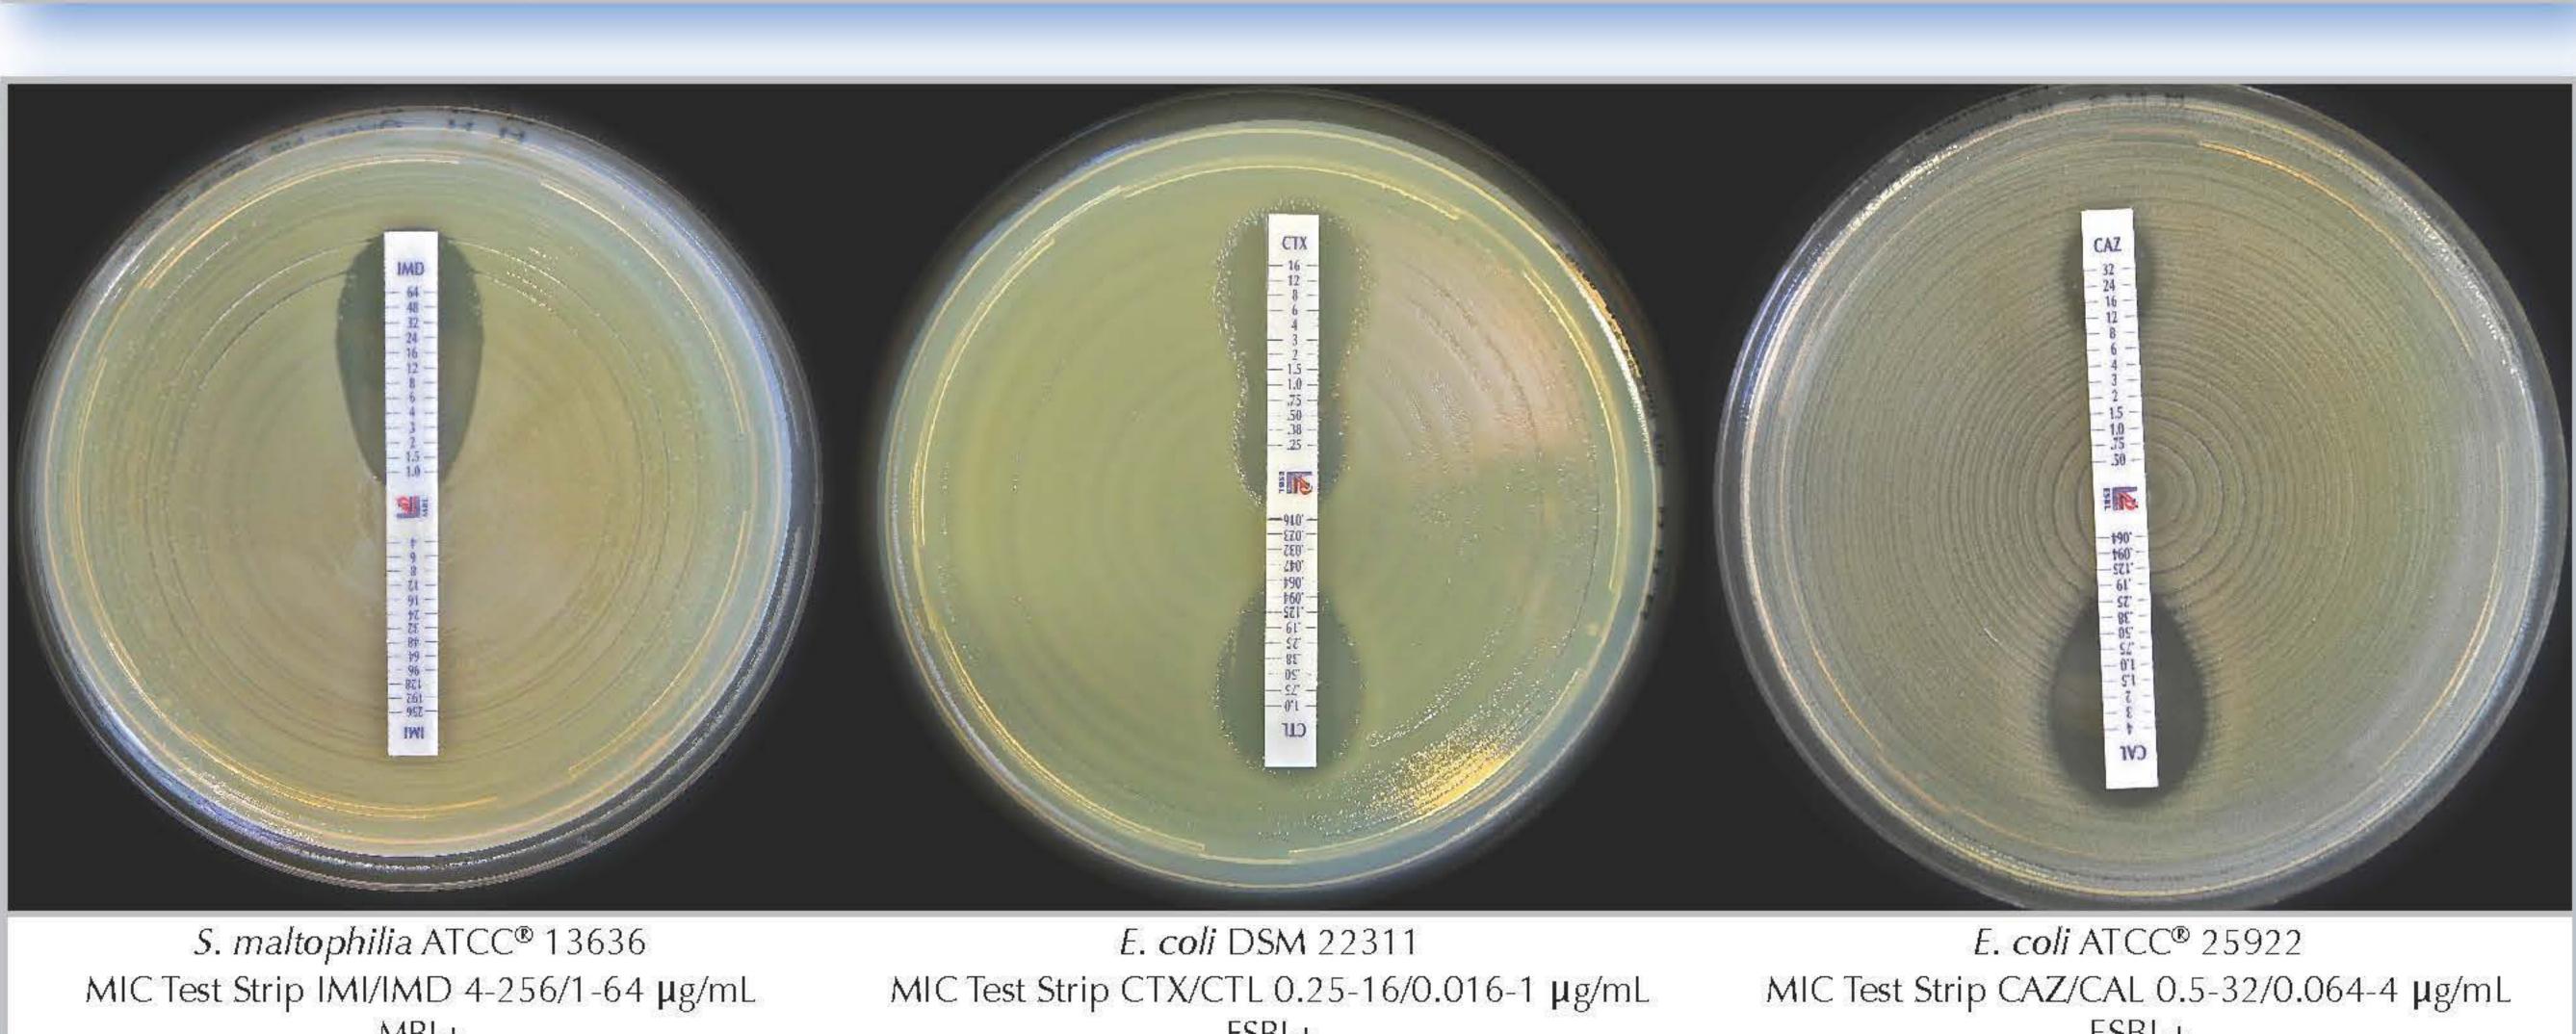

MBL+

ESBL+


ESBL+

## Contact your local dealer or Liofilchem headquarter for MIC Test Strip availability.



**Sarl Dimed** 

Tel +213 (0)21 75 53 80 Fax +213 (0)21 75 53 91 www.dimed-dz.com

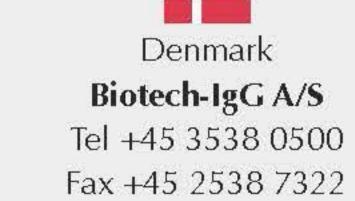

info@biotech-igg.com

Italy Liofilchem

Tel +39 0858930745 Fax +39 0858930330 www.liofilchem.it



Saudi Arabia Gamsco

Tel +966-3-8394085 Fax +966-3-8394084 drmalyousef@yahoo.com



MedicaTec S.R.L. Tel +54 11 4554.4600 Fax +54 11 4555.0416



**Media Medix Trade** Tel +20 22598417 Fax +20 24519256 mediamo\_co@yahoo.com



Japan

Alere Medical Co., Ltd. Tel +81353267393 Fax +81353267177 www.alere.co.jp



Serbia Uni-Chem

Tel +381113282986 Fax +381113281205 www.uni-chem.rs



www.medica-tec.com

Australia **Integrated Sciences Pty Ltd** 

Tel +61 2 9417 7866 Fax +61 2 9417 5066 www.integratedsci.com.au



Estonia

Borsa Eesti OÜ Tel +3725050555 Fax +3726556158

borsa@borsa.ee



Lithuania

Biometrija tel +37 052481824 fax +37 052400085 www.biometrija.lt



Singapore **Premier Diagnostics Pte Ltd** 

Tel +65 6220 3221 Fax +65 6220 9457 pdsingapore8@gmail.com



Belarus

Multi Lab Ltd. Tel.: +375 17 309 17 20 Fax: +375 17 299 09 02 multilab@multilab.by



Immuno Diagnostic Oy

Tel +3583615370

Fax +35836822039

www.immunodiagnostic.fi

Malaysia **Premier Diagnostics Sdn Bhd** 

Tel +603-8024-0680 Fax +603-8024-0780 www.premierdiagnostics.com.my



Slovakia


Bio G spol. s r.o. Tel +421245526381

Fax +421245526382 www.biog.sk



Benelux **ELITech Benelux B.V.B.A** 

Tel +32 (0)92820531 Fax +32 (0)92820532 c.notte@elitechgroup.com



France

Tel +33467504800 Fax +33467170906 www.i2a.info

i2a



New Zealand

**Point View Laboratories Ltd** 

Tel +64 9 533 3380 Fax +64 9 533 3340 info@pointviewlaboratories.com



Slovenia

Mediline d.o.o.

Tel +38618308050 Fax +38618308070 www.mediline.si



Elta 90M

Tel +35929839649 Fax +35929832211 www.elta90.com



Germany

bestbion dx GmbH Tel +49 2234 987 95 0 Fax +49 2234 987 95 29 bernd.stammel@bestbion.com



Norway **Montebello Diagnostics AS** 

Tel 22 14 14 90 Fax 22 14 44 90 www.montebello.no



South Africa

**Davies Diagnostics (PTY Ltd)** Tel +27117777600 Fax +27117876917

www.daviesdiagnostics.co.za



Alere Canada

Tel (613) 271-1144 Fax (613) 271-1148 www.alere.ca



Greece Varelas S.A.

Tel +302105281920 Fax +302105220926 microbiology@varelas.gr



Pakistan

**Imran Scientific Co** Tel 021-32210083

Fax 021-32210630 www.imransco.com




IZASA Distribuciones Técnicas, S.A.

Tel 902203090 Fax 902223366 www.izasa.es



Medica Tec de Chile S.A.

Tel +56 (02) 4261830 fax +56 (02) 4261835 mrojas@medica-tec.cl



Hungary Frank Diagnosztika Kft.

Tel 388-3114, 367-2430 Fax 368-5721 www.frank-diagn.hu



GT Scientific S.A.

Tel 595 21 200134 Fax 595 21 221339 ventas@gtscientific.com.py



Biotech-IgG AB

Tel +46 46 12 37 40 Fax +46 46 12 37 60 ak@biotech-igg.com



Croatia

**Tamiko Instruments** Tel +38514683046 Fax +38514684811 www.tamiko.hr



Indonesia

PT Suryana Microbiology Tel 62 21 345 2783 Fax 62 21 384 7232 najib@ptsuryana.com



Portugal

Izasa Portugal Distribuiçoes Tecnicas Lda. Tel +351 214161288 Fax +351 214176484 MIC Test Strip product range only



Thailand

Envimed Co., Ltd. Tel 66-2-434-0391 Fax 66-2-435-5962

envimed@truemail.co.th



Cuba

Tel 2041432-2041433 Fax 2040987 microbiologia@cpm.co.cu

CPM Cuba



Iran

Pishro Imen Pajouh Co.Ltd.

Tel +98 21 44328639 Fax + 98 21 44311632 pipco.ir@gmail.com



Romania

S.C. Sanimed International Impex SRL Tel 021.420.54.94 Fax 021.420.54.93 www.sanimed.ro



Turkey

Kemiteks Kimyevi Mad. Tic. Ltd. Sti. Tel +90 216 449 58 70 Fax +90 216 449 58 72 www.kemitekskimya.com.tr



United Kingdom **Launch Diagnostics Ltd** Tel +44(0)1474874426 Fax +44(0)1474872388

enquiries@launchdiagnostics.com



Czech Republic BioVendor

Tel +420549124123 Fax +420549211465 www.biovendor.cz



**Launch Diagnostics Ireland** 

Tel +3530719151122 Fax +3530719152277 desruddy@launchdiagnostics.ie



Agros-International, Zao

Tel +7 (812) 303-8234 Fax +7 (812) 303-8236 agros@agros-int.com





ref. 6553003 Rev.14.1 / 29.05.2014



